

## AMNIOQUICK®

Rapid test for detection of IGFBP-1 (Insulin Growth Factor Binding Protein 1)



### INTENDED USE

AMNIOQUICK® is a simple and rapid test that allows *in vitro* detection of IGFBP-1 (Insulin Growth Factor Binding Protein 1) from a vaginal swab sample. AMNIOQUICK® test is intended to detect the rupture of fetal membranes in pregnant woman with suspected rupture from a vaginal swab sample. Each test is used to obtain a visual result.

The AMNIOQUICK® Test Device can be used as an aid to initiate or attend therapeutic treatments by physicians. Each device is designed for professional and *in-vitro* diagnostic.

### INTRODUCTION

The Premature Rupture of Membranes or **PROM** is relatively frequent and concerns 5 to 10 % of pregnancy cases. It might lead to preterm delivery and fetal infection. The leakage of amniotic liquid is not always detectable by conventional clinical examination and therefore confirmatory biological test is sometimes useful. Biological tests are based on detection of alkalization of vaginal fluid (easy to proceed, sensitive, inexpensive but poorly specific) or presence of a molecule which is physiologically present in high concentration in amniotic fluid (diamine oxidase, alpha feto protein, fibronectin, IGFBP-1).

### TEST PRINCIPLE

A pair of monoclonal antibodies anti-IGFBP-1 is used for the IGFBP-1 detection. One is immobilized on the nitrocellulose membrane at the level of the test line: it corresponds to the capture antibody. Another one is labelled with colloidal gold for the subsequent revelation.

During the sample migration, IGFBP-1, if present in the sample, will form antigen-antibody complexes with the labelled antibodies. These complexes will be captured by the capture antibodies on the test line, creating one purple coloured line generated by gold nanoparticles.

The presence of a purple internal control line in the upper part of the membrane indicates that the result is valid and that the followed procedure is correct.

### MATERIAL PROVIDED

- Test strips individually pouched with a desiccant.
- Sterile Dacron vaginal swab.
- Unit dose vial of Diluent.
- Workstation (or rack tube).
- Instruction for use.

### MATERIAL REQUIRED BUT NOT PROVIDED

- Stop watch or timer.

### STORAGE AND STABILITY

AMNIOQUICK® test is packed in aluminium pouch with desiccant bag. The kit should be stored in a dry area at 2-30°C.

Under these conditions the strip is stable until the indicated expiry date. The strip must be protected from humidity. Once the pouch is open, the test should be performed within 1 hour maximum.

### PRECAUTIONS

- For diagnostic *in vitro* use only.
- For best results, strictly follow the test procedure and storage instructions.
- Do not open the foil pouch until it reaches room temperature to prevent formation of condensation. Humidity and high temperature can affect results.
- Do not use the kit beyond the expiration date.
- Do not eat, drink or smoke during the handling of the samples and the test.
- Do not pipet by mouth. Use white coat, disposable gloves and ocular protections while handling potentially infectious material and performing the assay.

- All patient samples should be handled as potentially infectious. When performing the test, all materials used should be treated as if they were potentially infectious. Then, eliminate the components of the test and the sample according to the suitable procedure for potentially infectious waste.
- Avoid splashes and aerosol formation. Clean up spills thoroughly using an appropriate disinfectant.
- Test strips provided in the kit are intended for single use. Do not re-use.
- Do not interchange or mix reagents from different kits and lots.
- Do not use a strip if the foil pouch is opened or damaged.

### SPECIMEN COLLECTION AND HANDLING

Use the sterile Dacron swab to collect secretions on the vaginal wall. Open the swab bag and place the swab into the vagina (5 cm depth) for 1 minute. Alternatively, speculum may be used and vaginal secretion may be collected by leaving the swab into contact with the vaginal wall at the level of the posterior fornix for 15 seconds, into the vagina (5cm depth) for 15 seconds. ~~Collection of sample from the cervix or from the posterior fornix should be avoided. The epithelial cells located in those zones may contain elevated levels of phosphorylated IGFBP-1 that may cross-react with the test.~~

### TEST PROCEDURE

- 1) Bring the complete kit and samples to be tested to room temperature prior to testing.
- 2) Open the unit dose vial and lay it vertically on a flat and horizontal surface.
- 3) Dip the swab into the unit dose vial and rotate for 10 seconds. Then discard the swab.
- 4) Dip the strip into the vial with arrows pointing downwards. Gently hit the dipstick on the bottom of the tube to enhance migration. Keep the strip in the tube in vertical position for 10 minutes.
- 5) Read the result after 10 minutes from the time the strip is dipped in the tube. **Do not interpret any Test band appearing 15 minutes after the strip is dipped in the vial.**
- 6) Then, eliminate the components of the test and the sample according to the suitable procedure for potentially infectious waste

### RESULTS INTERPRETATION

A proper reading requires:

- A minimum visual acuity,
- Good lighting conditions.

#### POSITIVE:



#### Presence of two distinct bands:

- A purple control line appears at the control line level.
  - A purple test line appears (even if intensity is weak) at the test line level.
- Presence of amniotic fluid in the sample.


#### NEGATIVE:



#### Only one band appears at the level of the control line C.

No band appears at the level of test line T.  
Amniotic fluid is not present in the sample.

#### INVALID:

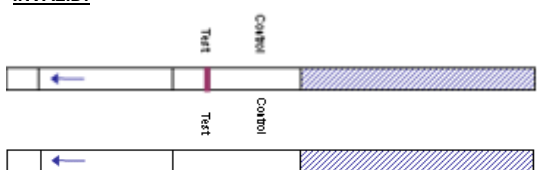

#### Absence of control line C.



Results from a test with no control line must be discarded.  
Review the procedure and repeat it with a new test device and a new tube.  
If the problem persists, contact your local distributor.

#### QUALITY CONTROL

- Internal procedural controls are included in the test. A coloured line appearing in the control zone (C) ensures that sufficient specimen volume has been loaded and that the correct procedure has been followed.
- Good Laboratory Practices recommend the use of positive and negative controls to check the correct test operating.  
Control samples specific for this product are available separately.

#### LIMITATIONS OF PROCEDURE

- As with all diagnostic tests, the test result must be consistent with clinical findings.
- False positive results might be linked to presence of IGFBP-1 coming from important bleeding or from decidual cells of the cervix when cervix is mature enough.
- False negative results might appear when test is performed more than 12 hours after the leakage of amniotic fluid has stopped.
- The swab has to be diluted in extraction tube immediately after collection of sample. Then the tube can be kept for 6 hours maximum at room temperature or 4°C before running the test as proteases in vaginal secretions may alter IGFBP1 if stored longer than 6 hours.

#### PERFORMANCES

##### Detection limit:

Detection limit of the AMNIOQUICK® test determined using a native IGFBP-1 control prepared in the test dilution buffer is **5 ng/ml**.

##### Clinical studies:

Different evaluations were achieved in a hospital environment to determine diagnostic efficacy of the AMNIOQUICK® test:

Site	Authors	Sensitivity	Specificity	Number of patients
<a href="#">Rochester NY, USA, 2011</a>	<a href="#">Newcomb and al.</a>	<a href="#">92.2%</a>	<a href="#">93.1%</a>	<a href="#">272</a>
<a href="#">Chaoyang hospital, Beijing 2010</a>	<a href="#">Li Yanfang and al.</a>	<a href="#">98.48%</a>	<a href="#">100%</a>	<a href="#">200</a>
<a href="#">Airlangga University, Indonesia 2013</a>	<a href="#">Arvati and al.</a>	<a href="#">85%</a>	<a href="#">95%</a>	<a href="#">52</a>
<a href="#">Chengdu University, China 2012</a>	<a href="#">Wang and al.</a>	<a href="#">80% 100% before 37 weeks</a>	<a href="#">100%</a>	<a href="#">200</a>

##### Hook effect:

Hook effect can be observed with AMNIOQUICK® test for concentrations above 500µg/mL of native IGFBP-1 diluted in the extraction tube. (The reference values for the IGFBP-1 amniotic concentration are between 10,5 and 350 µg/mL.)

#### Literature

1. Friedman ML, McElin TW. Diagnosis of ruptured fetal membranes. *Am J Obstet Gynecol* 1969;104:544-550
2. Steinman G, Kleiner GJ, Greston WM. Spontaneous rupture of membranes. *NY St. J Med* 1979;1849-1851
3. Koninckx PR, Trappeniers H, van Assche FA. Prolactin concentration in vaginal fluid: a new method for diagnosing ruptured membranes. *Br J Obstet Gynaecol* 1981;88:607-610
4. Rochelson BL, Richardson DA, Macri JN. Rapid assay: possible application in the diagnosis of premature rupture of the membranes. *Obstet Gynecol* 1983;62:414-418
5. Bell SC, Hales MW, Patel SR, Kirwan PH, Drife JO, Milford-Ward A. Amniotic fluid concentrations of secreted pregnancy-associated endometrial alpha1 and alpha2 globulins (alpha1 and alpha2 PEG). *Br J Obstet Gynaecol* 1986;93:909-915
6. Suikkari AM, Rutanen EM, Seppälä M. Circulating levels of immunoreactive insulin-like growth factor-binding protein in non-pregnant women. *Hum Reprod* 1987;2:297-300
7. Bell SC, Keyte JW; N-terminal amnio acid sequence of human pregnancy-associated endometrial alpha1-globulin, an endometrial insulin-like growth factor (IGF) binding protein – Evidence for two small molecular weight IGF binding proteins. *The Endoc Soc* 1988:1202-1204
8. Rutanen EM, Pekonen F, Kärkkäinen T. Measurement of insulin-like growth factor binding protein-1 in cervical/vaginal secretions: comparison with the ROM-check membrane immunoassay in the diagnosis of ruptured fetal membranes. *Clin Chim Acta* 1993;214:73-81
9. Medina TM, Hill DA. Preterm premature rupture of membranes: diagnosis and management. *Am Fam Physic* 2006;73: 659-664
10. Lockwood CJ, Wein R, Chien D, Ghidini A, Alvarez M, Berkowitz RL. Fetal membrane rupture is associated with the presence of insulin-like growth factor-binding protein-1 in vaginal secretions. *Am J Obstet Gynecol* 1994;171:146-150
11. Guibourdenche J, Luton D, André E, Noël M, Porquet D. Détection rapide de l'Insulin-like growth factor-binding protein-1 et de la fibronectine fœtale dans les sécrétions cervico-vaginales pour le diagnostic de la rupture prématurée des membranes. *Ann Clin Biochem* 1999 ;36 :388-390

12. Sucak A, Moroy P, Cakmak P, Mungan T, Mollamahmutoglu L, Danisman N. Insulin-Like Growth Factor Binding Protein-1; a rapid detection of amniotic fluid leakage after amniocentesis. *Turk J Med Sci* 2005;35:157-161

13. Talabani H, Recoules A, Grenier S, Luton D, Paper T, Porquet D, Oury JF, Guibourdenche J. L'alpha1-microglobuline placentaire dans les sécrétions vaginales : un nouveau marqueur de la rupture prématurée des membranes. *Act Pharm Biol Clin* 2005 ;12 :233-240

14. Akercan F, Cirpan T, Kazandi M, Terek MC, Mgoji I, Ozkinay E. The value of insulin-like growth factor binding protein-1 in the cervical-vaginal secretion detected by immunochromatographic dipstick test in the prediction of delivery in women with clinically unconfirmed preterm premature rupture of membranes. *Eur J Obstet Gynecol Rep Biol* 2005;121:159-163

#### SYMBOLS:



Attention, see instructions for use



Lot number



For *in vitro* diagnostic use only



Manufacturer



Store between 2-30°C



Do not reuse



Tests per kit



Catalog number



Expiry



Diluent



**BIO SYNEX**

12, rue Ettore Bugatti – CS28006  
67038 STRASBOURG Cedex – France

Tél. : +33 3 88 77 57 00  
Fax : +33 3 59 81 21 74

[info@biosynex.com](mailto:info@biosynex.com)  
[www.biosynex.com](http://www.biosynex.com)

Page 2/2

**BIO SYNEX**

Version 056 EN 03/2015